


TEST REPORT

(Electronic version)

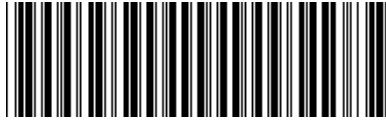

No:200156943

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: WPRQ-1150-04

ISSUE DATE:2020-06-04

扫码下载报告



APPLICANT: YU-HUANG ELECTRONICS DONGGUAN CO., LTD.
ADDRESS: ROOM 101 OF BUILDING 4, NO. 3 OF TUTANG INDUSTRIAL ROAD, CHANGPING TOWN, DONGGUAN CITY, GUANGDONG PROVINCE

INFORMATION CONFIRMED BY APPLICANT:

KN95 MASK
QUANTITY: 60 PIECES
STYLE NO.: 20200513
SIZE: 5205288

DATE RECEIVED/DATE TEST STARTED: 2020-06-04

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
VISUAL FIELD	M
HEAD BAND	M
FLAMMABILITY	M
APPEARANCE INSPECTION[2 PIECES]	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" -NO COMMENT

REMARK:

THE AUTHORIZATION OF APPEARANCE INSPECTION IS NOT RECEIVED FROM CNAS.
THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200128368.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

ZiShan Guo SENIOR ENGINEER

郭子山




PAGE 1 OF 4

TEST REPORT

(Electronic version)

No:200156943

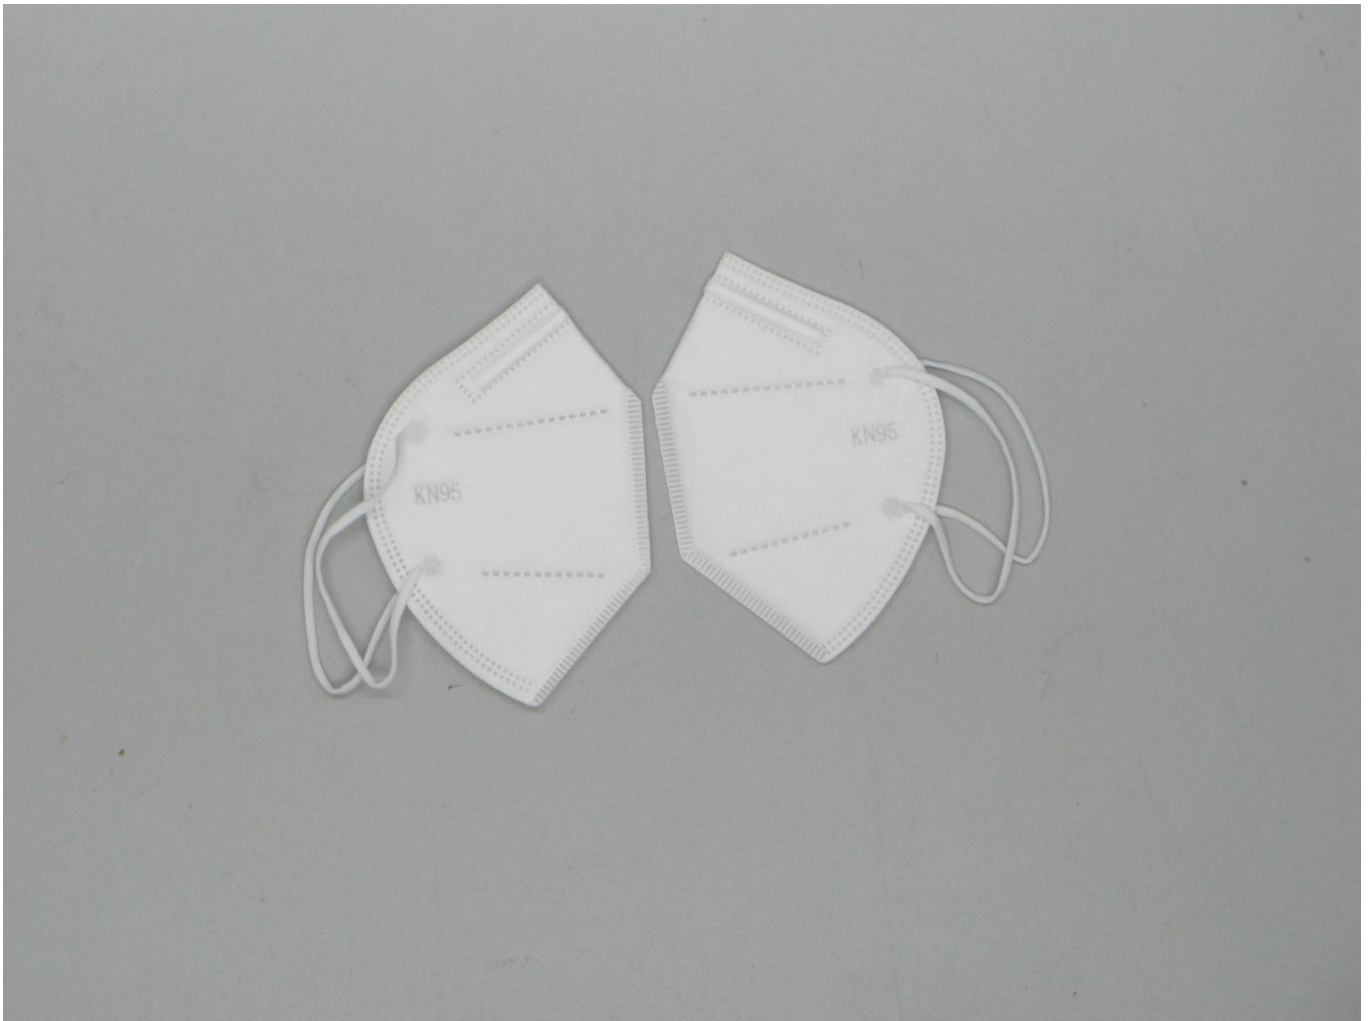

TEST REPORT

(Electronic version)

No:200156943

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER(%)

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m³, TEMP:23.7℃ RH:36.6%)

FILTRATION EFFICIENCY:
UNTREATED SAMPLE

1# 98.57
2# 98.43
3# 98.92
4# 98.30
5# 98.41
6# 97.98
7# 98.06
8# 98.11
9# 98.55
10# 98.48

CONDITIONING TREATED

1# 98.12
2# 97.86
3# 97.92
4# 98.34
5# 98.41

REQUIREMENT

FILTRATION EFFICIENCY:
≥95.0
(KN95)
(GB 2626-2006)

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 108.8
2# 100.2

PRETREATMENT SAMPLE:

1# 93.6
2# 94.2

REQUIREMENT

≤350
(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 130.9
2# 131.2

PRETREATMENT SAMPLE:

1# 103.2
2# 104.3

REQUIREMENT

≤250
(GB 2626-2006)

VISUAL FIELD(°)

(GB 2890-2009 6.8)

65

REQUIREMENT

≥60
(GB 2626-2006)

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:

1# PASS

CONDITIONING TREATED:

1# PASS

REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUSTING PARTS OF MASK SHOULD NOT SLIP OR BREAK UNDER 10N TENSION FOR 10S.
(GB 2626-2006)



PAGE 3 OF 4

TEST REPORT

(Electronic version)

No:200156943

FLAMMABILITY(s)

(GB 2626-2006 6.15)

AFTERFLAME TIME
UNTREATED SAMPLE
1# 0.0
2# 0.0
CONDITIONING TREATED
3# 0.0
4# 0.0

REQUIREMENT
AFTERFLAME TIME
≤5
(GB 2626-2006)

APPEARANCE INSPECTION[2 PIECES]

(GB 2626-2006 6.1)

PASS

REQUIREMENT
ACCORDING TO THE CLAUSE 5.2 OF THE
PRODUCT STANDARD
(GB 2626-2006)



————End of Report————

PAGE 4 OF 4